

EL-GFX-VAC2



Dual Channel High Accuracy Thermistor Glycol Probe Data Logger with Graphic Screen

- -40 to +125°C (-40 to +257°F) measurement range
- Stores over 250,000 readings
- Logging rates between 2 seconds and 1 hour
- On screen menu and graphing to start, stop, review and restart the logger in the field
- Triggered logging mode to start recording data once a user defined level is met
- High contrast, greyscale, backlit, graphic LCD screen to denote status and alarm levels
- User-programmable audible alarm thresholds with highly visible confidence/alarm LEDs
- EasyLog software available as a free download



This standalone data logger measures and stores over 250,000 temperature readings over a -40 to +125°C (-40 to +257°F) range at a resolution of 0.1°C (0.2°F).

The user can easily set up the logger and view downloaded data by plugging the data logger into a PC's USB port and using the available free downloadable EasyLog software. Data can then be graphed, printed and exported to other applications.

The data logger features a high contrast dot-matrix LCD and three buttons to navigate through an on-screen menu. This menu provides the user with access to real-time trend analysis, data summaries and the ability to start, stop and restart the data logger without the need to connect the data logger to the host-PC. Users can reset the maximum / minimum reading using the on-screen menu. This introduces an 'event marker' into the data which can later be viewed in the graphing software ('Mark Events' option) and the data file after download.

The data logger is supplied complete with two lithium metal batteries, which can typically allow logging for up to 4 months.

SPECIFICATIONS

Type 2 Probe <i>(Supplied)</i>	Measurement Range	-40 to 125°C (-40 to 257°F)
	Accuracy (-10 to 70°C / 14 to 158°F)	±0.3°C (±0.5°F)
	Accuracy (-40 to 125°C / -40 to 257°F)	±1°C (±1.8°F)
Accuracy (Logger error)		±0.1°C (±0.2°F)
Internal Resolution		0.1°C (0.2°F)
Logging Rate		Every 2 seconds to 1 hour
Operating temperature Range		-10 to 40°C (14 to 104°F)
2X 1/2 AA 3.6V Lithium Battery Life		4 months
Dimensions		101 x 48.5 x 30.5mm (3.97 x 1.90 x 1.20")

ACCESSORIES

BAT 3V6 1/2AA	Replacement battery (2 required)
EL-P-VAC	Replacement thermistor glycol probe

INCLUDED IN THE BOX

x2 BAT 3V6 1/2AA	Battery
CABLE USB A-MICRO B	USB cable
EL-GFX WALL BRACKET	Magnetic mounting bracket
x2 EL-P-VAC	Thermistor glycol probes
CAL-TEMP-UK	Temperature Calibra- tion certificate



CALIBRATION CERTIFICATES INCLUDED

The EL-GFX-VAC2 comes with a calibration certificate issued at 2 and 8°C, using reference equipment which has been calibrated by a UKAS/NIST accredited laboratory and using apparatus traceable to national or international standards. For more information, please see www.lascarelectronics.com.



EL-GFX-VAC2




Dual Channel High Accuracy Thermistor Glycol Probe Data Logger with Graphic Screen

EL-WIN-USB

Lascar's EasyLog control software is available as a free download from www.easylogusb.com. Easy to install and use, the control software is compatible with 32-bit and 64-bit versions of Windows 7, 8 and 10. The software is used to set up the logger, download, graph and annotate data or export in Excel, PDF and jpeg formats.

The software allows the following parameters to be configured:

- Logger name
- Measurement parameter (°C or °F)
- Logging rate (user selectable between 2 seconds and 1 hour)
- Display off, on for 30 seconds after button press, or permanently on
- High and low alarms
- Disable or enable LEDs and sounder with delayed activation
- Immediate, delayed, triggered and push-to-start logging

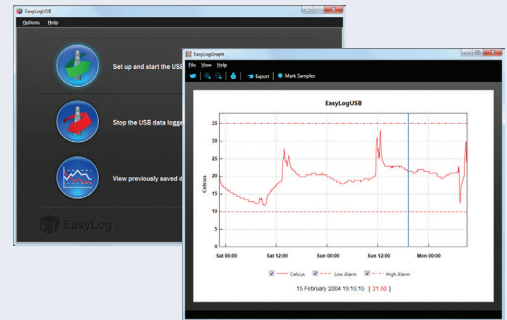

Download the latest version of the software free of charge from www.easylogusb.com

MENU BUTTON FUNCTIONS AND LCD SCREEN INDICATION

<p>ARMED! Press button to start logging</p> <p>DELAYED START Starts logging at 10:30:00 04/03/12</p> <p>DELAYED START Starts logging when temperature above 36.2°C</p>	<p>START LOGGER</p> <ul style="list-style-type: none"> • Loggers can be started immediately on a button press, delayed to a specific time or delayed to specific temperature reading 		<p>DISPLAY DATA</p> <ul style="list-style-type: none"> • Data can be displayed on screen in tabular or graphical format • You can switch between these views by pressing the gfx / txt buttons at the bottom-left of your screen
<p>ON-SCREEN ICONS</p> <div style="display: flex; justify-content: space-around;"> <div data-bbox="183 1400 327 1534"> <ul style="list-style-type: none"> • When the EasyLog cube is shown in the top-left corner your logger is logging </div> <div data-bbox="375 1400 518 1534"> <ul style="list-style-type: none"> • High/Low Alarm indicators are displayed at the top of your screen </div> <div data-bbox="646 1400 758 1534"> <ul style="list-style-type: none"> • This icon indicates that your battery is low and will need to be replaced soon </div> </div>		<p>STOP/START LOGGING & MUTE ALARM</p> <div style="display: flex; justify-content: space-around;"> <div data-bbox="821 1377 949 1512"> <p>⊙ Stop Logging ○ Logger Settings</p> </div> <div data-bbox="949 1377 1077 1512"> <p>⊙ Start Logging ○ Logger Settings</p> </div> <div data-bbox="1077 1377 1212 1512"> <p>⊙ Mute Alarm ○ Stop Logging ○ Logger Settings</p> </div> </div> <ul style="list-style-type: none"> • By pressing the stop button, you can stop your logger, or view logger settings. If you have already stopped logging, this option will change to 'Start Logging'. The audible alarm can be muted from this menu if enabled 	
<p>SUMMARY DATA</p> <div style="display: flex; justify-content: space-around;"> <div data-bbox="191 1579 327 1702"> <p>Temperature Max 34.8°C Min 22.8°C Since 10:30 24/09/2012</p> </div> <div data-bbox="327 1579 454 1702"> <p>Mem Used 32% Readings 6336</p> </div> </div> <ul style="list-style-type: none"> • Summary screen displays max/min log and last log. Reset function clears summary if required • These screens can be reached by pressing the i button 		<p>LOCKED MODE</p> <ul style="list-style-type: none"> • When in locked mode - an option during PC set-up - the logger can only be stopped and re-started using a PC loaded with the unit's configuration software 	
<p>LOGGER SETTINGS</p> <div style="display: flex; justify-content: space-around;"> <div data-bbox="191 1736 327 1848"> <p>○ Start Logging ⊙ Logger Settings</p> </div> <div data-bbox="327 1736 454 1848"> <p>EasyLog USB Sample Rate 10s Low Alm 10°C High Alm 40°C S/N 000000001</p> </div> </div> <ul style="list-style-type: none"> • To view a summary of the logger's settings press the stop button, then click 'Logger Settings' 		<p>POP-UP MESSAGES</p> <div style="display: flex; justify-content: space-around;"> <div data-bbox="821 1736 949 1848"> <p>Time & date not set Start unit logging using PC</p> </div> <div data-bbox="949 1736 1077 1848"> <p>Memory is 90% full Download data to a PC to clear</p> </div> <div data-bbox="1077 1736 1212 1848"> <p>Memory full, logger stopped Download data to a PC to clear</p> </div> </div> <ul style="list-style-type: none"> • A message will overlay the screen - if there is an issue - the next time a button is pressed, e.g. if the logger is running low on memory 	


Please note that screens may vary slightly depending on model.

EL-GFX-VAC2



Dual Channel High Accuracy Thermistor Glycol Probe Data Logger with Graphic Screen

PROBE MEASUREMENT ACCURACY

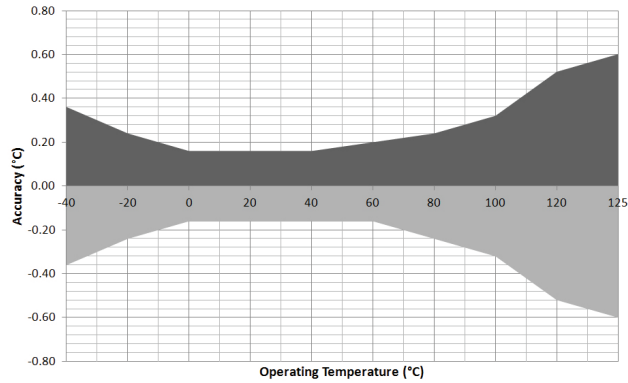

BATTERY INFORMATION

Replacement

We recommend that you replace the battery every year, or prior to logging critical data. Only use 3.6V ½AA lithium batteries. The data logger does not lose its stored readings when the battery is discharged or replaced; however, the data logging process will stop and will not resume until the battery is replaced and the logger restarted by EL-WIN-USB.

Before replacing the battery, remove the data logger from the PC. Please note that leaving the data logger plugged into the USB port for extended periods will cause some of the battery capacity to be lost.

Passivation

If left unused for extended periods of time, lithium batteries including those used in the EasyLog range of data loggers naturally form a non-conductive internal layer, preventing them from self-discharge and effectively increasing their shelf life. When first installed in the data logger, this may cause a momentary drop in the battery voltage (the Transient Minimum Voltage) as the internal layer is broken down, resulting in the data logger resetting. Inserting the batteries in the data logger and leaving it connected to a PC for about 30 seconds will remove this layer. After this, remove and re-install the batteries to reset the data logger. Overall battery life will not be affected.

WARNING

Handle lithium batteries carefully, observe warnings on battery casing. Dispose of in accordance with local regulations.